ANALIZA BIAŁEK

Scan for verify

100019714

Laboratory of Analysis

Client: Veriphase
Order number: 100019714
Name: VERIPHASE CJC-1295 NO DAC IPAMORELIN
Number of samples: 1 vial

Batch number: 26-0042
Receive date: 2026-10-26
Start date: 2026-10-27
End date: 2026-10-28

Sample identification

Substance	Method of taking a sample	Form
CJC-1295 no DAC, Ipamorelin	Sample provided by customer	White powder in a glass vial

Results

Substance	Sample name	Content	Purity
CJC-1295 no DAC	VERIPHASE CJC-1295 NO DAC IPAMORELIN 5MG+5MG	4,50mg	99%
Ipamorelin	VERIPHASE CJC-1295 NO DAC IPAMORELIN 5MG+5MG	5,25mg	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, peaks of the sought substances appeared. Their contents, when compared to the reference chromatograms, are shown in the table above. Height the measurement error is +-0,05mg. The actual state of the sample sent before the test is presented on the photo below.

Photo of the test sample



Password

UIWE9XON

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA


Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając

ANALIZA BIAŁEK

Scan for verify

100019714

Chromatogram

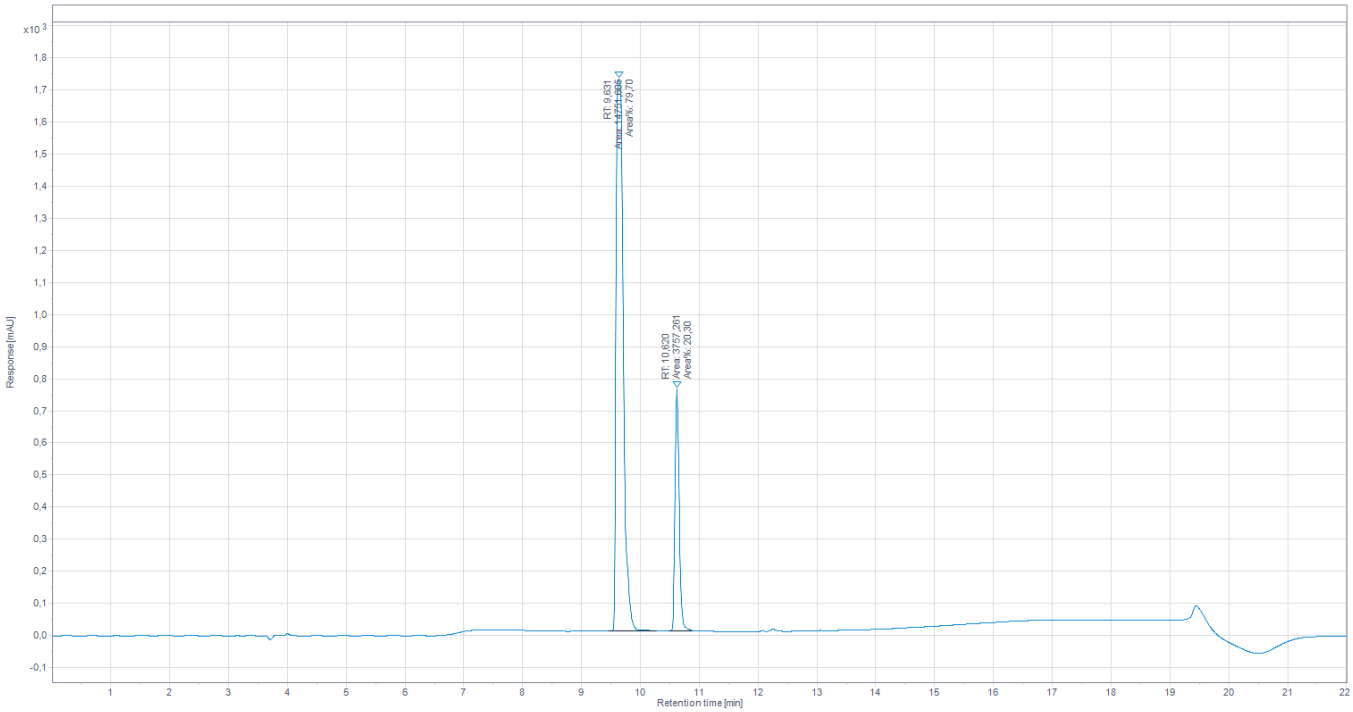

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

UIWE9XON

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając